


MSA: Ferritin

CLSI EP15-A3 - Table 8

Last updated 10 August 2018 at 12:24 by Simon

Descriptives

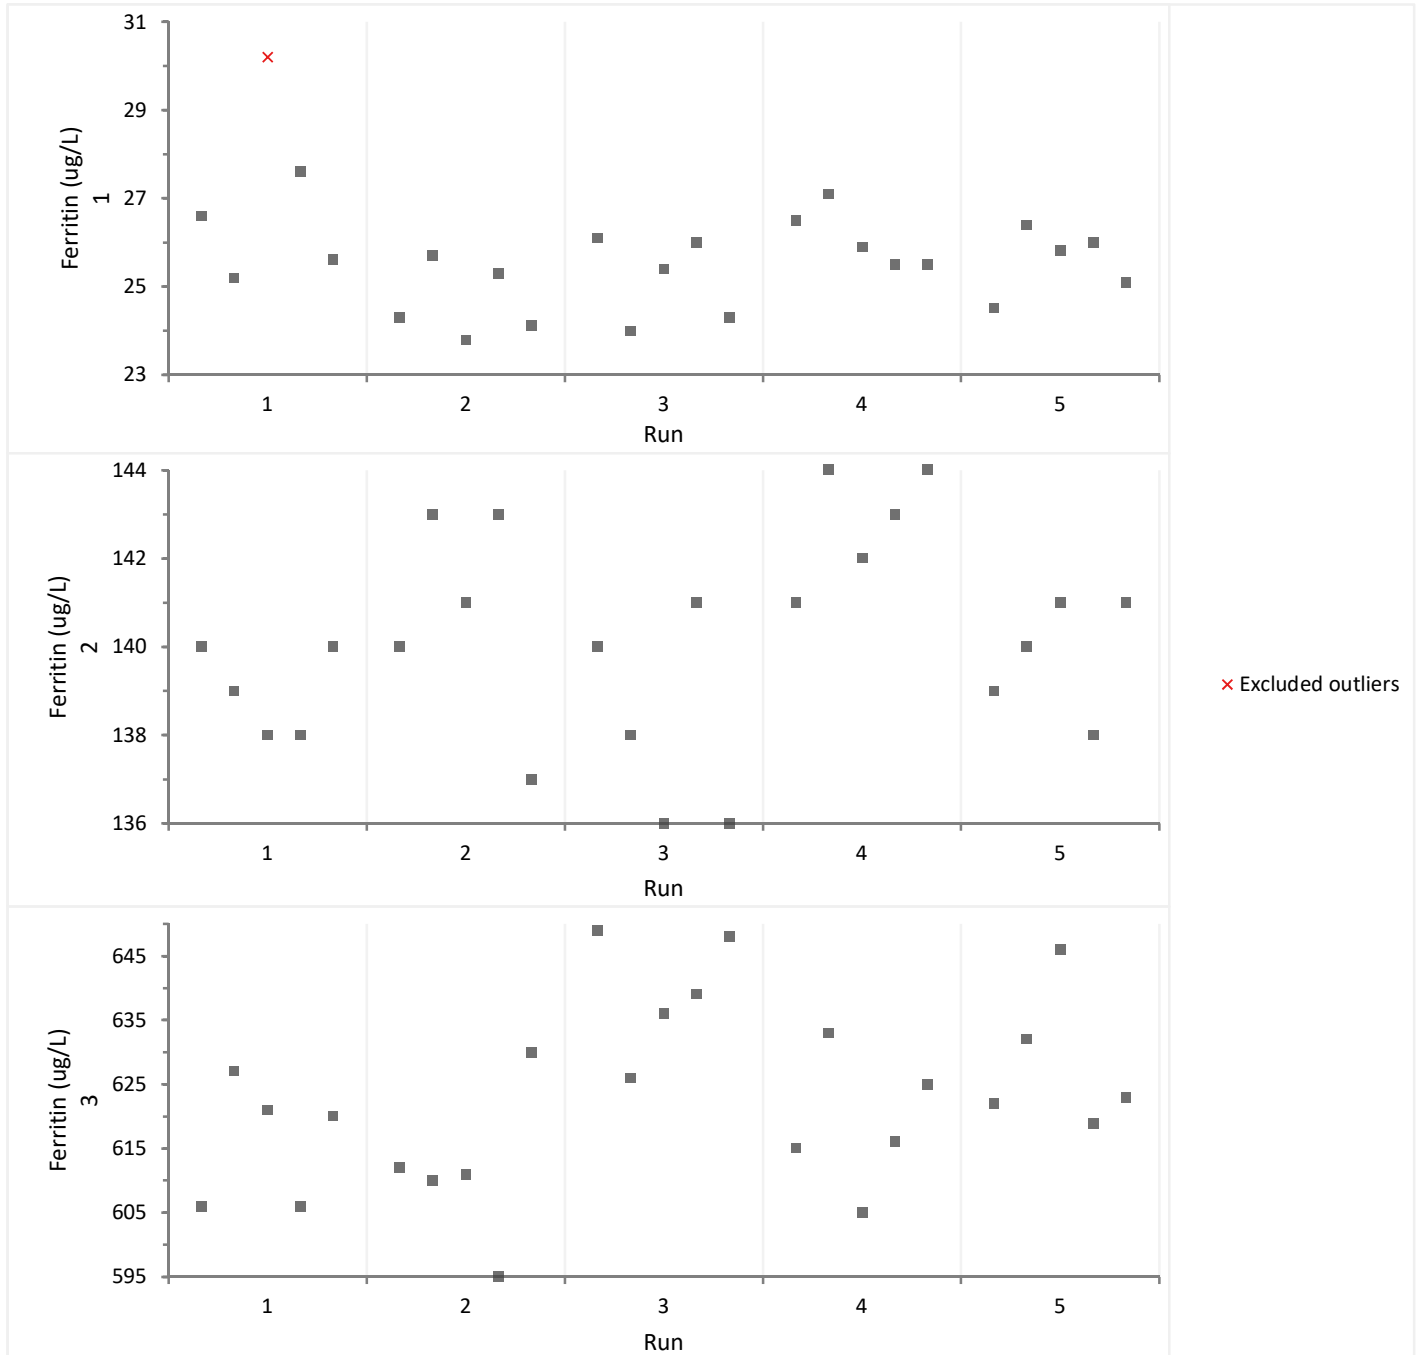

MSA: Ferritin

CLSI EP15-A3 - Table 8

Last updated 10 August 2018 at 12:24 by Simon

Sample, Run, #	Outlier #	Outlier	Mean	SD	Z	Critical value
1, 1, 3	1	30.2	25.70	1.35	3.34	3.14

Outliers excluded from analysis.

N	74
Design	3 Sample x 5 Run x 5 Observations

Unequal number of observations for all possible combinations of factor levels.

Measuring interval	25.51 to 622.88
--------------------	-----------------

MSA: Ferritin

CLSI EP15-A3 - Table 8

Last updated 10 August 2018 at 12:24 by Simon

Precision

Sample	Mean	Within Run SD	Within Run CV	Total SD	Total CV
1	25.51	0.86	3.4%	1.01	4.0%
2	140.12	1.78	1.3%	2.39	1.7%
3	622.88	10.65	1.7%	14.70	2.4%

Sample 1

Component	SD	CV	Expected SD / CV	p-value
Within Run	0.86	3.4%	3.3%	0.4023 ¹
Between Run	0.53	2.1%		
Total	1.01	4.0%	5.3%	0.9154 ¹

H0: $\sigma \leq \sigma_0$

The imprecision is less than or equal to the expected imprecision.

H1: $\sigma > \sigma_0$

The imprecision is greater than the expected imprecision.

¹ Do not reject the null hypothesis at the 5% familywise (1.67% individual) significance level.

X² test

	SD	Expected SD	X ² statistic	DF	p-value
Within Run	0.86	0.84	19.87	19	0.4023
Total	1.01	1.35	8.91	16.0	0.9154

ANOVA

Source	Type I SS	DF	MS	Expected MS
Run	8.34	4	2.09	$\sigma_{Error}^2 + 4.792\sigma_{Run}^2$
Error	14.09	19	0.74	σ_{Error}^2

MSA: Ferritin

CLSI EP15-A3 - Table 8

Last updated 10 August 2018 at 12:24 by Simon

Sample 2

Component	SD	CV	Expected SD / CV	p-value
Within Run	1.78	1.3%	2.0%	0.9915 ¹
Between Run	1.59	1.1%		
Total	2.39	1.7%	3.4%	0.9945 ¹

H0: $\sigma \leq \sigma_0$

The imprecision is less than or equal to the expected imprecision.

H1: $\sigma > \sigma_0$

The imprecision is greater than the expected imprecision.

¹ Do not reject the null hypothesis at the 5% familywise (1.67% individual) significance level.

X² test

	SD	Expected SD	X ² statistic	DF	p-value
Within Run	1.78	2.80	8.05	20	0.9915
Total	2.39	4.76	2.88	11.5	0.9945

ANOVA

Source	SS	DF	MS	Expected MS
Run	63.44	4	15.86	$\sigma_{\text{Error}}^2 + 5\sigma_{\text{Run}}^2$
Error	63.20	20	3.16	σ_{Error}^2

MSA: Ferritin

CLSI EP15-A3 - Table 8

Last updated 10 August 2018 at 12:24 by Simon

Sample 3

Component	SD	CV	Expected SD / CV	p-value
Within Run	10.65	1.7%	1.6%	0.2958 ¹
Between Run	10.13	1.6%		
Total	14.70	2.4%	2.8%	0.7265 ¹

H0: $\sigma \leq \sigma_0$

The imprecision is less than or equal to the expected imprecision.

H1: $\sigma > \sigma_0$

The imprecision is greater than the expected imprecision.

¹ Do not reject the null hypothesis at the 5% familywise (1.67% individual) significance level.


X² test

	SD	Expected SD	X ² statistic	DF	p-value
Within Run	10.65	9.97	22.86	20	0.2958
Total	14.70	17.44	7.65	10.8	0.7265

ANOVA

Source	SS	DF	MS	Expected MS
Run	2506.24	4	626.56	$\sigma_{\text{Error}}^2 + 5\sigma_{\text{Run}}^2$
Error	2270.40	20	113.52	σ_{Error}^2

Descriptives

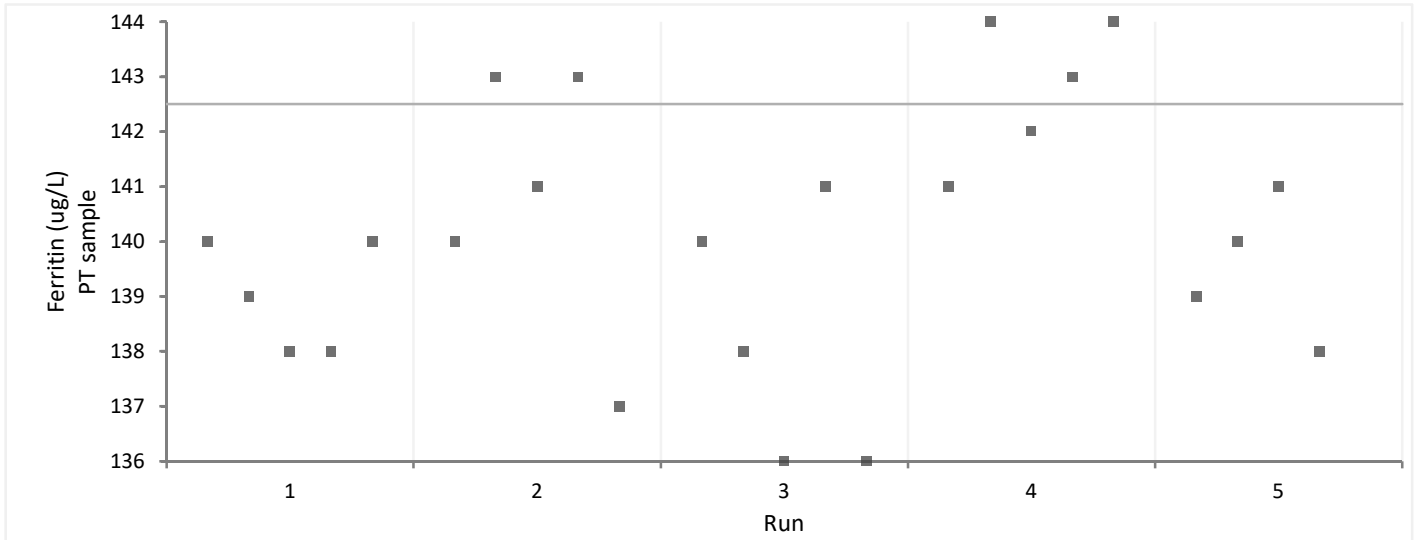


N | 24
 Design | 5 Run x 5 Observations

Unequal number of observations for all possible combinations of factor levels.

	Assigned value	Uncertainty SE	DF
PT sample	142.5	0.69	42

	N	Mean	Mean SE	Recovery
PT sample	24	140.1	0.82	98.3%

Trueness

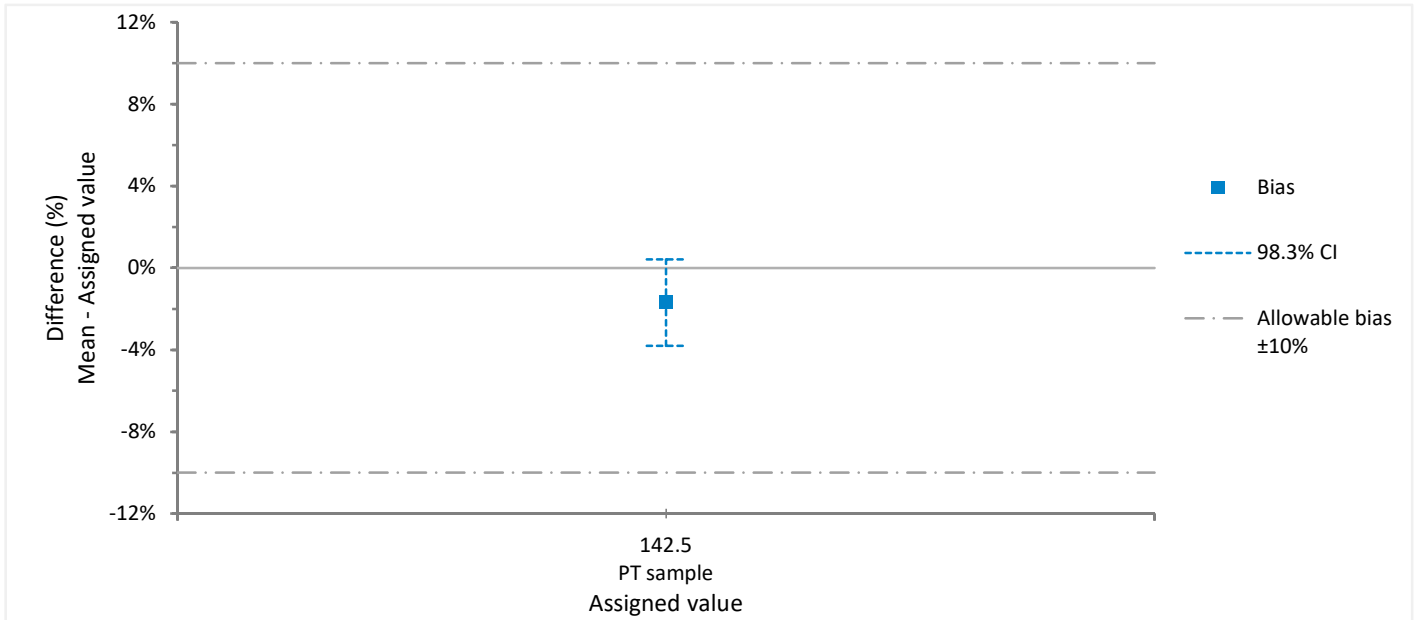

Assigned value	Mean	Bias	98.3% CI	Allowable bias	p-value
142.5	140.1	-1.7%	-3.8% to 0.4%	±10.0%	0.0456 ¹

H0: $\delta = 0$

The bias is equal to 0.

H1: $\delta \neq 0$

The bias is not equal to 0.

¹ Do not reject the null hypothesis at the 1.67% significance level.

Student's t-test

Assigned value	Difference	SE	t statistic	DF	p-value
142.5	-2.4	1.1	-2.25	11.1	0.0456